

Document made available under the Patent Cooperation Treaty (PCT)

International application number: PCT/IL05/000871

International filing date: 11 August 2005 (11.08.2005)

Document type: Certified copy of priority document

Document details: Country/Office: US
Number: 60/619,792
Filing date: 19 October 2004 (19.10.2004)

Date of receipt at the International Bureau: 01 December 2005 (01.12.2005)

Remark: Priority document submitted or transmitted to the International Bureau in compliance with Rule 17.1(a) or (b)



World Intellectual Property Organization (WIPO) - Geneva, Switzerland
Organisation Mondiale de la Propriété Intellectuelle (OMPI) - Genève, Suisse

10 NOV 2005

PA 1370986


THE UNITED STATES OF AMERICA**TO ALL TO WHOM THESE PRESENTS SHALL COME:****UNITED STATES DEPARTMENT OF COMMERCE****United States Patent and Trademark Office****September 23, 2005**

**THIS IS TO CERTIFY THAT ANNEXED HERETO IS A TRUE COPY FROM
THE RECORDS OF THE UNITED STATES PATENT AND TRADEMARK
OFFICE OF THOSE PAPERS OF THE BELOW IDENTIFIED PATENT
APPLICATION THAT MET THE REQUIREMENTS TO BE GRANTED A
FILING DATE UNDER 35 USC 111.**

APPLICATION NUMBER: 60/619,792**FILING DATE: October 19, 2004**

**By Authority of the
Under Secretary of Commerce for Intellectual Property
and Director of the United States Patent and Trademark Office**

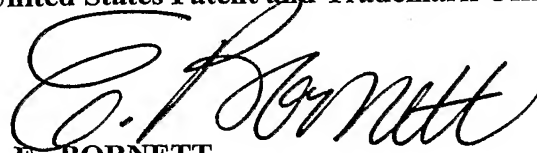


E. BORNETT
Certifying Officer

16523 U.S. PTO

Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.
Approved for use through 07/31/2006. OMB 0651-0032
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE

PROVISIONAL APPLICATION FOR PATENT COVER SHEET

This is a request for filing a PROVISIONAL APPLICATION FOR PATENT under 37 CFR 1.53(c).

Express Mail Label No.

INVENTOR(S)					
Given Name (first and middle [if any])		Family Name or Surname		Residence (City and either State or Foreign Country)	
SHLOMI		BEN ARI		BINYAMINA ISRAEL	
Additional inventors are being named on the _____ separately numbered sheets attached hereto					
TITLE OF THE INVENTION (500 characters max)					
USING A CATHETER OR GUIDEWIRE TRACKING SYSTEM TO PROVIDE POSITIONAL FEEDBACK FOR AN AUTOMATED CATHETER OR GUIDEWIRE NAVIGATION SYSTEM					
Direct all correspondence to: CORRESPONDENCE ADDRESS					
<input type="checkbox"/> Customer Number: _____					
OR					
<input checked="" type="checkbox"/> Firm or Individual Name		SHLOMI BEN ARI			
Address		POB 368			
Address					
City		BINYAMINA		State	
Country		ISRAEL		Zip	30550
		Telephone	0097246380881	Fax	
ENCLOSED APPLICATION PARTS (check all that apply)					
<input checked="" type="checkbox"/> Specification Number of Pages 6		<input type="checkbox"/> CD(s), Number _____			
<input type="checkbox"/> Drawing(s) Number of Sheets _____		<input type="checkbox"/> Other (specify) _____			
<input type="checkbox"/> Application Data Sheet. See 37 CFR 1.76					
METHOD OF PAYMENT OF FILING FEES FOR THIS PROVISIONAL APPLICATION FOR PATENT					
<input type="checkbox"/> Applicant claims small entity status. See 37 CFR 1.27.				FILING FEE Amount (\$)	
<input type="checkbox"/> A check or money order is enclosed to cover the filing fees.				160	
<input type="checkbox"/> The Director is hereby authorized to charge filing fees or credit any overpayment to Deposit Account Number: _____					
<input checked="" type="checkbox"/> Payment by credit card. Form PTO-2038 is attached.					
The invention was made by an agency of the United States Government or under a contract with an agency of the United States Government.					
<input checked="" type="checkbox"/> No.					
<input type="checkbox"/> Yes, the name of the U.S. Government agency and the Government contract number are: _____					

17513 U.S. PTO
60/619792

101904

Respectfully submitted,

[Page 1 of 2]

Date 5 October 2004

SIGNATURE



REGISTRATION NO. _____

(if appropriate)

TYPED or PRINTED NAME SHLOMI BENARI

Docket Number: _____

TELEPHONE 00972-4-6380881

USE ONLY FOR FILING A PROVISIONAL APPLICATION FOR PATENT

This collection of information is required by 37 CFR 1.51. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 8 hours to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. SEND TO: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.

If you need assistance in completing the form, call 1-800-PTO-9199 and select option 2.

PROVISIONAL APPLICATION COVER SHEET
Additional Page

PTO/SB/16 (04-04)

Approved for use through 07/31/2006. OMB 0651-0032

U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE

Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

Docket Number

INVENTOR(S)/APPLICANT(S)

Given Name (first and middle [if any])	Family or Surname	Residence (City and either State or Foreign Country)

[Page 2 of 2]

Number _____ of _____

WARNING: Information on this form may become public. Credit card information should not be included on this form. Provide credit card information and authorization on PTO-2038.

Using a catheter or guidewire tracking system to provide positional feedback for an automated catheter or guidewire navigation system

Provisional Patent

Written by:
Shlomi Ben-ari

Table of Contents

1. Scope	3
2. Background	3
3. The invention	4
3.1. Overview	4
3.2. Preferred Embodiment	4

Table of Figures

Figure 1 - Example of system display during navigation with elements labeled	5
Figure 2 - System Block Diagram with indication of data flow	6

1. Scope

This application provides a description of a novel medical catheterization method based on utilizing a guidewire and/or catheter tracking system to provide position feedback to an automated guidewire or catheter navigation system. It is written in order to be submitted as a provisional patent.

2. Background

Although catheter tracking systems have been in existence for a number of years using a number of different technologies (RF tracking, magnetic tracking, MR Tracking, MRI gradient field tracking, etc...) they have generally been used for special purpose tracking (i.e. cardiac mapping), and not for aiding in navigation during catheterization. This is most likely because the navigation during catheterization is performed primarily with a guidewire and the existing catheter tracking technologies require a tracked element which is too large to be placed on a standard guidewire.

Guidewire and catheter navigation is generally guided by fluoroscopy. This is true for manual catheterization as well as for automated navigation systems such as the magnet driven Niobe navigation system produced by Stereotaxis Inc.

The use of a tiny radioactive source as the tracked element in a catheter or guidewire tracking system, as described in the provisional patent entitled "Utilizing a radioactive source as the tracked element for a tracking system", makes it possible to use such a tracking system as the primary guiding system for the navigation of a guidewire or catheter. Using such a tracking system instead of fluoroscopy has the potential to significantly reduce the radiation dose to the patient and practitioner during intravascular procedures.

3. The invention

3.1. Overview

The invention disclosed here is the use of a guidewire or catheter tracking system as the primary guiding system for an automated catheter or guidewire navigation system. The automated navigation system is capable of applying a force in any direction upon the tip of the guidewire, but in order to navigate the guidewire, it needs real-time feedback about the position of the tip of the guidewire. Current automated navigation systems, such as the Stereotaxis Niobe system, use fluoroscopy to provide this feedback. In addition to being inherently two dimensional (and therefore requiring extra time and processing to produce 3-dimensional information), fluoroscopy guidance results in a high radiation dose to the patient. Replacing the fluoroscopy guidance in such automated navigation systems with a 3-dimensional guidewire tip tracking system will provide real-time 3-dimensional tip position feedback with significantly reduced radiation dose.

3.2. Preferred Embodiment

The system consists of an automated catheter/guidewire navigation system, a C-arm fluoroscopy system (for visualization of the intravascular procedure once navigation to the target location has been completed, blood flow diagnostics, initial 3-D angiography, etc...), and a 3-dimensional guidewire and/or catheter tracking system.

A 3-dimensional angiography data set will either be provided from previous MRI or CT angiography, or will be produced at the outset of the procedure using the fluoroscopy system.

The 3-dimensional angiography data set will be used to produce a 3-dimensional model of the vasculature within which the system will navigate.

The target will then be indicated by the doctor on the 3-dimensional model and the route to the target will be either automatically or manually determined. Once the guidewire is brought into the region of the 3-dimensional vasculature model, the automated navigation system will pull the tip of the guidewire along the predetermined route based on real-time position feedback from the tracking system.

The navigation system computer will control the direction in which the navigation system pulls the guidewire tip at each point in time based on the current tip position provided by the tracking system and the predetermined route on the 3-dimensional vasculature model.

The use of the tracking system for position feedback will reduce both procedure time and radiation dose compared to fluoroscopy guidance.

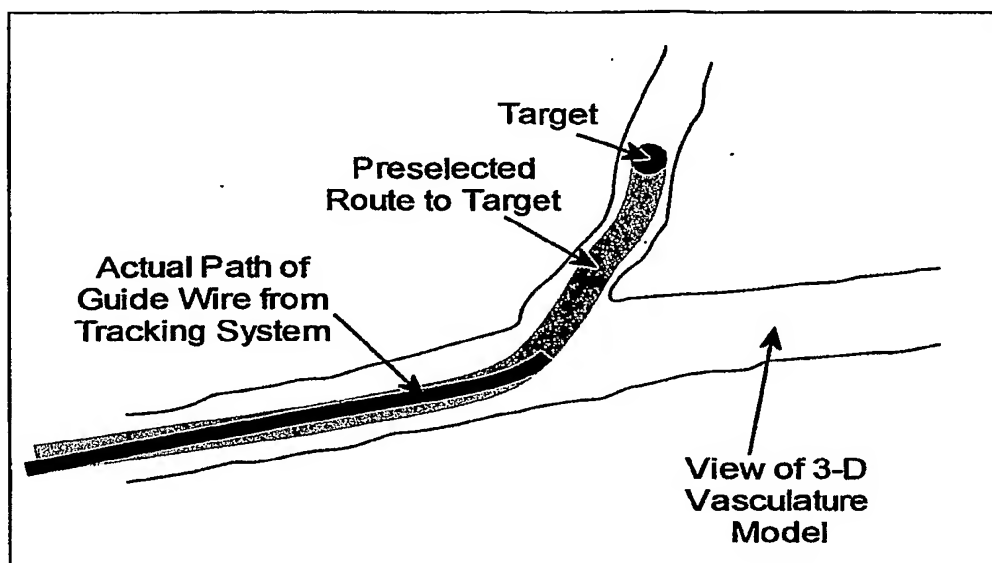


Figure 1 - Example of system display during navigation with elements labeled

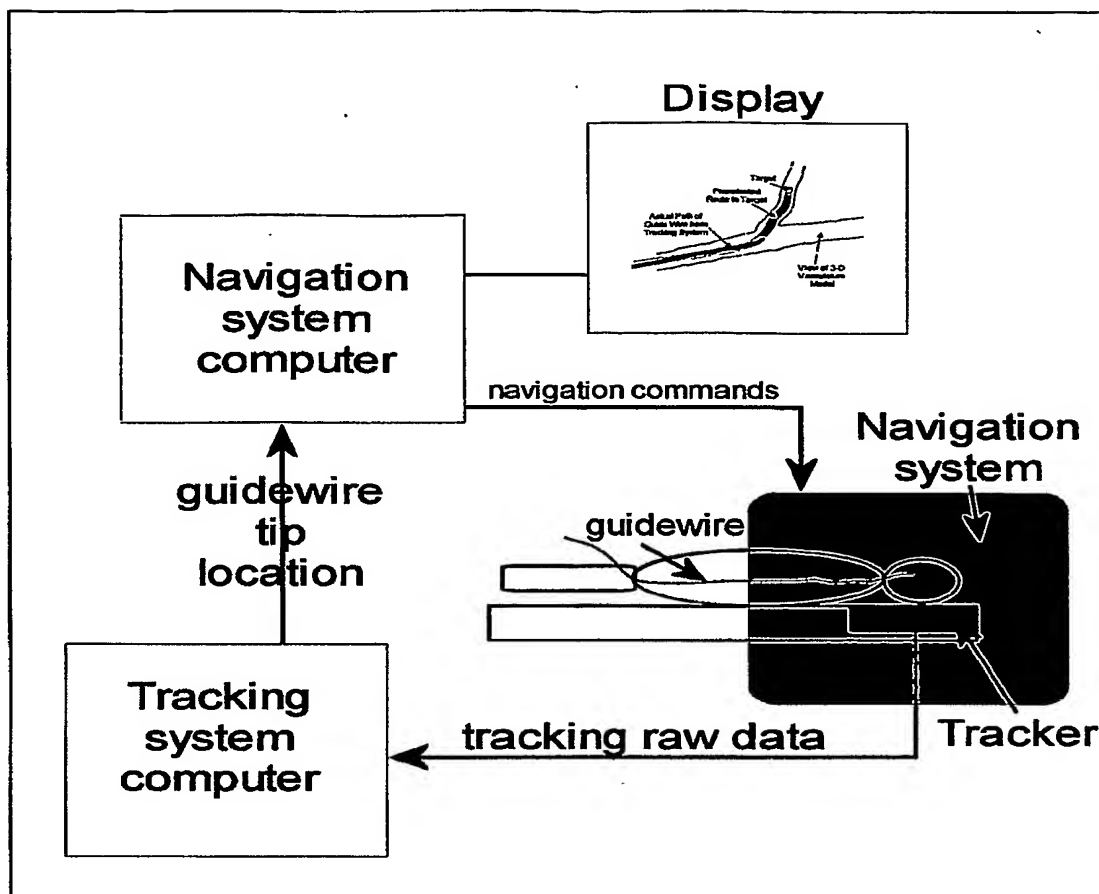


Figure 2 - System Block Diagram with indication of data flow